


PCT

WORLD INTELLECTUAL PROPERTY ORGANIZATION
International Bureau

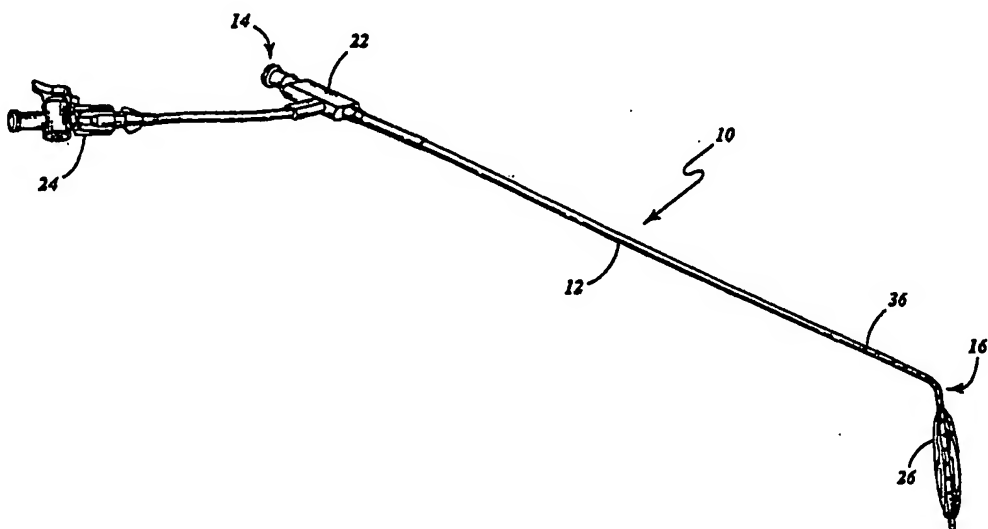

INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁶ : A61B 5/02	A1	(11) International Publication Number: WO 00/10452 (43) International Publication Date: 2 March 2000 (02.03.00)
(21) International Application Number: PCT/US99/17406 (22) International Filing Date: 30 July 1999 (30.07.99) (30) Priority Data: 09/137,949 21 August 1998 (21.08.98) US (71) Applicant: AGA MEDICAL CORP. [US/US]; 682 Mendelssohn Avenue, Golden Valley, MN 55427 (US). (72) Inventors: AMPLATZ, Kurt; 10 Evergreen Road, St. Paul, MN 55127 (US). AFREMOV, Michael, R.; 1664 Virginia Avenue South, St. Louis Park, MN 55426 (US). (74) Agent: DIETZ, Paul, T.; Nikolai, Mersereau & Dietz, P.A., Suite 820, 900 Second Avenue South, Minneapolis, MN 55402-3325 (US).		(81) Designated States: AU, CA, CN, JP, KR, Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE). Published <i>With international search report.</i>
(54) Title: SIZING CATHETER FOR MEASURING SEPTAL DEFECTS  (57) Abstract <p>This invention is a sizing catheter (10), and method of measuring a preselected internal opening within a patient to provide a rapid, precise determination of a stretched diameter of the preselected internal opening. The sizing catheter (10) includes a dilation balloon (26) constructed of a thin expandable plastic which is inflatable, and is utilized to determine a size of the preselected opening. The dilation balloon (26) is inflated to an inflation threshold, wherein the dilation balloon (26) deforms about the preselected opening, and the size of the dilation balloon (26) adjacent the preselected opening approximates a stretched diameter of the preselected opening. The sizing catheter (10), and method may be utilized to determine an appropriate sized occluding device to thereby occlude the preselected opening.</p>		

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece	ML	Mali	TR	Turkey
BG	Bulgaria	HU	Hungary	MN	Mongolia	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MR	Mauritania	UA	Ukraine
BR	Brazil	IL	Israel	MW	Malawi	UG	Uganda
BY	Belarus	IS	Iceland	MX	Mexico	US	United States of America
CA	Canada	IT	Italy	NE	Niger	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NL	Netherlands	VN	Viet Nam
CG	Congo	KE	Kenya	NO	Norway	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NZ	New Zealand	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	PL	Poland		
CM	Cameroon	KR	Republic of Korea	PT	Portugal		
CN	China	KZ	Kazakhstan	RO	Romania		
CU	Cuba	LC	Saint Lucia	RU	Russian Federation		
CZ	Czech Republic	LI	Liechtenstein	SD	Sudan		
DE	Germany	LK	Sri Lanka	SE	Sweden		
DK	Denmark	LR	Liberia	SG	Singapore		
EE	Estonia						

SIZING CATHETER FOR MEASURING SEPTAL DEFECTS

BACKGROUND OF THE INVENTION.

I. FIELD OF THE INVENTION

The present invention relates generally to a device and non-surgical method for
5 determining the size of an internal opening within a patient. More particularly, the present
invention relates to a sizing catheter and method of using the same, wherein the sizing catheter
may be utilized to determine the stretched diameter of an internal passage within a patient.
The sizing catheter of the present invention is particularly well suited for determining the
stretched diameter of a defect, such as a septal defect, within the heart of a patient. Once the
10 stretched diameter of the defect is known, a properly sized occluding device may be selected
and positioned within the opening of the defect.

II. DESCRIPTION OF THE RELATED ART

Over the years various medical devices, including stents and occluders, have been
developed for placement within a preselected internal passage, opening, or defect of a patient.
15 Complex devices may be delivered and used in treating specific abnormal conditions, such as
devices used in removing vascular occlusions or devices used in treating septal defects and the
like. Through advancement in a variety of devices, stents and occluders may be delivered non-
surgically. Certain intravascular devices, such as catheters and guide wires, may be used to
deliver certain medical devices to a specific location within a patient's heart, for example.
20 Further, a catheter may be used to reach a selected coronary artery within the vascular system
or a catheter and/or guidewire may be used to deliver a device to an interior chamber of the
patient's heart.

Prior to delivering the particular medical device, the size of the internal passage,
opening or defect must be determined in order that an appropriately sized device may be
25 provided. Further, determination of the "stretched diameter" of the opening or defect is
desirable to provide a preferred fit between the medical device and the surrounding tissue. In
the past, physicians have utilized a balloon catheter in an attempt to determine the size of the
internal opening or defect. Typically, the physician will position the balloon within the
opening and slowly inflate the balloon, pushing or pulling the balloon of the catheter fore or
30 aft until the physician feels resistance against the balloon. The size of the balloon
corresponding with the size of the opening is then determined. The technique of pulling or

pushing a balloon catheter through the opening or defect is unreliable and does not determine the size of the opening when the surrounding tissue is stretched.

A balloon catheter and a calibrated guidewire having radiopaque regions of known length, may be utilized by a physician during a preliminary fluoroscopic procedure to estimate the defect's size, shape and thickness of the septal wall near the defect. Although useful, the defects exact size when stretched and the shape cannot be determined, thereby increasing the possibility of leakage around the device.

Echocardiography has also been used to estimate the diameter of the opening or defect, however, echo measurements are always significantly smaller than the "stretched diameter". The differences between echo measurements and stretched diameters may range between 2mm to 10.5mm. It has been suggested that the stretched diameter can be estimated from echo measurements by multiplying 1.05 times the echo measurement and then adding 5.49. Although this formula may prove sufficient in some cases, differences of up to 4.5mm between the actual stretched diameter and the estimated diameter from this formula have been observed. The errors in echo measurements can be explained by the fact that most communications are not perfectly round whereas the balloon transforms the deformed communication into a round structure. If a device is selected which is too small, the risk of embolization and residual shunting increases significantly. On the other hand, if the device is too large, the device may not fit properly within the opening or defect.

Other methods have been described for determining the size of the internal opening utilizing a balloon catheter. For example, Taheri et al. in U.S. Patent No. 5,591,195 describes a sizing catheter, wherein the pressure within an inflatable balloon is measured. Taheri et al. teaches that when the balloon makes contact with a vessel to be measured, the pressure within the balloon increases. The size of the balloon may then be determined from a chart of known balloon pressures and diameters. As seen in Figure 9, the pressure within the balloon may vary even though the actual diameter being measured remains the same. A need therefore exists for a device that can determine the stretched diameter of an internal passage, opening or defect. The present invention meets these and other needs which will become apparent to those skilled in the art.

SUMMARY OF THE INVENTION

The purpose of the present invention is to provide a device and method for

determining the nominal and/or "stretched diameter" of an internal opening or defect within a patient. Those skilled in the art will appreciate that the device and method of the present invention may be utilized to determine the size of any of several defects, passages, or internal openings within a patient. For ease of discussion, and without any limitation intended, the device and method of the present invention will be described in conjunction with determining the stretched diameter of a septal defect within the heart of a patient.

The device and method of the present invention may be utilized in conjunction with radiology, fluoroscopy, echocardiography, and/or other known suitable means for viewing the distal end of a catheter positioned within a patient's heart. The sizing catheter of the present invention includes a tubular shaft having a longitudinal axis extending between a proximal end and a distal end of the tubular shaft. The tubular shaft has one or more lumens formed within the tubular shaft, wherein the lumens are adapted for receiving, for example, a guidewire, device, pressurized fluid, etc. One of the lumens extends between the proximal end and a region short of the distal end of the tubular shaft and terminates into a series of ports extending through the tubular shaft from the lumen to an outer surface of the tubular shaft. The series of ports may be aligned in a spiral fashion around the circumference of the tubular shaft. An elongated dilation balloon is affixed to the tubular shaft proximate the distal end of the tubular shaft and encloses the series of ports.

The dilation balloon is constructed of a thin expandable plastic having an inflation threshold which corresponds with the stretchability of the tissue of the defect. In use, when the dilation balloon is positioned within the predetermined opening and inflated, the dilation balloon resists deformation up to the inflation threshold, thereby causing the tissue surrounding the opening to stretch. Once the inflation threshold is reached, the dilation balloon deforms about the predetermined opening, such that a noticeable waist of the balloon is formed adjacent the predetermined opening. Markings on the distal end of the catheter having known separation distances may be utilized to determine a size of the dilation balloon adjacent the predetermined opening, thereby assisting in the determination of the stretched diameter of the predetermined opening.

Alternatively, when the inflation threshold is reached and the dilation balloon deforms, the pressure within the dilation balloon may be noted. The catheter may then be removed from the heart and the distal end inserted in a template having apertures of known dimension.

The balloon may then be inflated to the noted pressure within an aperture estimated to be larger than the stretched diameter of the septal defect. If the balloon deforms, the selected aperture in the template may approximate the stretched diameter of the septal defect. The next size larger aperture may be tested to verify that the balloon does not deform in this larger aperture. If the balloon does not deform in the first selected aperture, then the next smaller aperture in the template is selected and the balloon is inflated to the noted pressure. If the balloon deforms in this aperture, the dimension of the aperture corresponds with the stretched diameter of the opening. This procedure is repeated until the balloon deforms within an aperture at the noted pressure. In this manner, the stretched diameter of the defect or passage may be determined.

In order to increase the likelihood that the distal end of the catheter extends through the defect perpendicular to the plane of the defect, the distal end of the tubular shaft may be preset with a 45 degree bend relative to the longitudinal axis of the tubular shaft. Those skilled in the art will appreciate that an angulation of 45 degrees relative to the longitudinal axis of the tubular shaft is preferable because the average atrial septum of the heart has a 45 degree inclination. Also, such orientation is preferrable when using the radiopaque markings to estimate distances and sizes within the heart.

OBJECTS

It is accordingly a principal object of the present invention to provide a device and method for non-evasively determining the size of a stretched internal passage or defect.

Another object of the present invention is to provide a device suitable for use in determining a properly sized occluding device for use occluding a defect.

These and other objects, as well as these and other features and advantages of the present invention will become readily apparent to those skilled in the art from a review of the following detailed description of the preferred embodiment in conjunction with the accompanying claims and drawings in which like numerals in the several views refer to corresponding parts.

BRIEF DESCRIPTION OF THE DRAWINGS

Figure 1 is a perspective view of a sizing catheter of the present invention;

Figure 2 is a partial sectional end elevational view of the catheter body of the present invention;

Figure 3 is a fragmented perspective view of the distal end of the sizing catheter of the present invention;

Figure 4 is a fragmented perspective view of the distal end of the sizing catheter of the type shown in Figure 3 with the balloon inflated;

5 Figure 5 is a fragmented perspective view of the distal end of the sizing catheter of the type shown in Figure 3 with the balloon inflated and positioned within an aperture of a sizing template;

10 Figure 6 is a fragmented perspective view of the distal end of the sizing catheter of the type shown in Figure 3 with the balloon inflated and positioned within a septal defect of a heart; and

Figure 7 is a chart demonstrating differences in the accuracy of determining the inflated size of the balloon of the sizing catheter of the present invention for several measuring means.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT

Referring first to Figure 1 there is shown generally a sizing catheter 10 for measuring
15 the size of a passage, opening, or defect. The sizing catheter 10 includes a tubular shaft 12 having a longitudinal axis extending between a proximal end 14 and a distal end 16 and includes a first and second lumen 18 and 20 formed therein. The proximal end includes a guidewire connector 22 and pressure valve assembly 24 coupled thereto. Without any limitation intended, in the preferred embodiment the first lumen 18 is adapted for receiving a
20 guidewire (not shown) therein. The second lumen 20 is formed within the tubular shaft 12 and extends between the proximal end 14 of the tubular shaft 12 to a region short of the distal end 16 and terminates into a series of ports 28 extending through the tubular shaft 12 from the lumen 20 to an outer surface of the tubular shaft 12 (see Figure 2). An elongated dilation
25 balloon 26 is affixed to the tubular shaft 12 proximate the distal end of the tubular shaft and encloses the series of ports 28 (see Figure 3). The second lumen 20 serves as a conduit between the balloon 26 and a means of known suitable construction for increasing the pressure within lumen 20 which is coupled to the pressure valve assembly 24. The first lumen 18 of the sizing catheter 10 may be sized for passage over a 0.035 inch guidewire, leaving room for a relatively large second lumen 20 for rapid inflation and deflation of the balloon 26.

30 The dilation balloon 26 is constructed of a thin expandable plastic having an inflation threshold, such that when the dilation balloon 26 is positioned and inflated within a

predetermined opening, the dilation balloon resists deformation up to the inflation threshold. Without any limitation intended, in the preferred embodiment the tubular shaft may be constructed of a known suitable radiopaque nylon based polymer composite and the balloon 26 may be constructed of a 2 mil thick expandable polymer such as a polyurethane membrane. Once the dilation threshold is reached, the dilation balloon 26 deforms about the predetermined opening. A size of the dilation balloon adjacent the predetermined opening approximates a stretched diameter of the predetermined opening.

Referring to Figure 4, the distal end 16 of the sizing catheter 10 is shown. Radiopaque markings 36 of known suitable construction may be affixed or formed on the tubular shaft 12 proximate the dilation balloon 26. The distal end 16 of the tubular shaft 12 is bent at a 45 degree angle relative to the longitudinal axis of the tubular shaft. In this manner the longitudinal axis of the distal end 16 of the sizing catheter 10 may be positioned perpendicular to the plane of the predetermined opening.

Referring to Figure 5, the distal end 16 of the sizing catheter 10 is shown positioned within an aperture 32 of template 30 with the balloon 26 inflated above the inflation threshold. Various sized apertures 32 of known dimension are formed in the template 30. As further described below, the pressure within the balloon inflated to the inflation threshold varies depending upon the size of the aperture 32.

Having described the constructional features of the present invention, the mode of use will next be described in conjunction with Figures 6 and 7. Those skilled in the art will appreciate that the device and method of the present invention may be utilized to determine the size of any of several defects, passages, or internal openings within a patient, however, for ease of discussion, and without any limitation intended, the mode of use will be described in conjunction with determining the stretched diameter of a septal defect within the heart of a patient. In the preferred embodiment, although it may not be necessary, prior to inserting the catheter within the patient, the balloon 26 is inflated with carbon dioxide and then all gases are aspirated from the second lumen 20.

After the hemodynamic data of the patient is obtained, an introducing catheter is passed through the atrial communication into one of the left pulmonary veins and an exchange guidewire is introduced. The introducing catheter and sheath are then removed and the sizing catheter 10 is passed over the exchange guidewire directly through the skin. To facilitate this

percutaneous entry, an assistant applies forceful negative pressure with an attached syringe. Under fluoroscopic and echocardiographic guidance, the distal end 16 of the sizing catheter 10 is positioned across the defect. The balloon 26 is then inflated with diluted contrast medium until a waist can be observed (the inflation threshold is reached) and/or left-to-right shunting ceases as observed by Doppler echocardiography. The diameter of the balloon 26 adjacent the defect may then be determined by many of several known means including echocardiography or radiology. Referring to the chart shown in Figure 7, it is anticipated that echo measurements will suffice, however, x-ray measurements can be added. Further, if desired, the sizing catheter 10 may be removed, and positioned within various apertures of template 30. The balloon is re-inflated with the same known amount of contrast medium, and it may be determined which aperture corresponds with the same deformation of the balloon 26 observed within the defect. Once the stretched diameter of the septal defect is determined, a properly sized occluding device may be selected positioned within the defect.

This invention has been described herein in considerable detail in order to comply with the Patent Statutes and to provide those skilled in the art with the information needed to apply the novel principles and to construct and use embodiments of the example as required. However, it is to be understood that the invention can be carried out by specifically different devices and that various modifications can be accomplished without departing from the scope of the invention itself.

What is claimed is:

CLAIMS

1. A sizing catheter for measuring the size of an intracardiac opening, said sizing catheter including: a tubular shaft having a longitudinal axis extending between a proximal end and a distal end thereof, said tubular shaft further having a lumen extending between the proximal end and a region short of the distal end and terminating into a series of ports extending through the tubular shaft from the lumen to an outer surface of the tubular shaft, wherein an elongated dilation balloon affixed to the tubular shaft proximate the distal end of the tubular shaft encloses the series of ports, said dilation balloon being constructed of a thin expandable plastic and having an inflation threshold, wherein when the dilation balloon is positioned within the predetermined opening and inflated, said dilation balloon resists deformation up to the inflation threshold such that when the inflation threshold is reached the dilation balloon deforms about the predetermined opening and a size of the dilation balloon adjacent the predetermined opening approximates a stretched diameter of the predetermined opening.

2. The sizing catheter as recited in claim 1, further including radiopaque markings affixed to the tubular shaft proximate the dilation balloon.

3. The sizing catheter as recited in claim 1, wherein the distal end of the tubular shaft is bent at a 45 degree angle relative to the longitudinal axis of the tubular shaft.

4. The sizing catheter as recited in claim 1, wherein the dilation balloon is constructed of an expandable polymer.

5. The sizing catheter as recited in claim 1, wherein the dilation balloon is constructed of polyurethane.

6. The sizing catheter as recited in claim 1, wherein the series of ports are aligned in a spiral fashion around the circumference of the tubular shaft.

7. A method of determining a size of an intracardiac opening, said method

including the steps of:


- a) providing a sizing means for sizing a predetermined internal opening of a patient, said sizing means including an elongated dilation balloon being constructed of a thin expandable plastic and being inflatable to thereby approximate a size of the predetermined opening;
- b) providing a viewing means for viewing the internal position of the elongated dilation balloon positioned within a patient's body;
- c) positioning the dilation balloon of the sizing means within the predetermined opening;
- d) inflating said dilation balloon to an inflation threshold, such that the dilation balloon deforms about the predetermined opening and a size of the dilation balloon adjacent the predetermined opening approximates a stretched diameter of the predetermined opening; and
- e) determining the size of the dilation balloon adjacent the predetermined opening.


8. The method as recited in claim 7, wherein the step of positioning the dilation balloon further includes positioning a longitudinal axis of the balloon relatively perpendicular to a plane of the predetermined opening.

9. The method as recited in claim 7, wherein said sizing means includes markers viewable by said viewing means, wherein said sizing means is advanced through the predetermined opening such that said markers may be utilized to determine a thickness dimension of the predetermined opening.

10. The method as recited in claim 8, wherein said sizing means includes markers viewable by said viewing means, wherein said sizing means is advanced through the predetermined opening such that said markers may be utilized to determine a thickness dimension of the predetermined opening.

11. The method as recited in claim 7, wherein the viewing means utilizes echocardiography to view the internal position of the elongated dilation balloon.

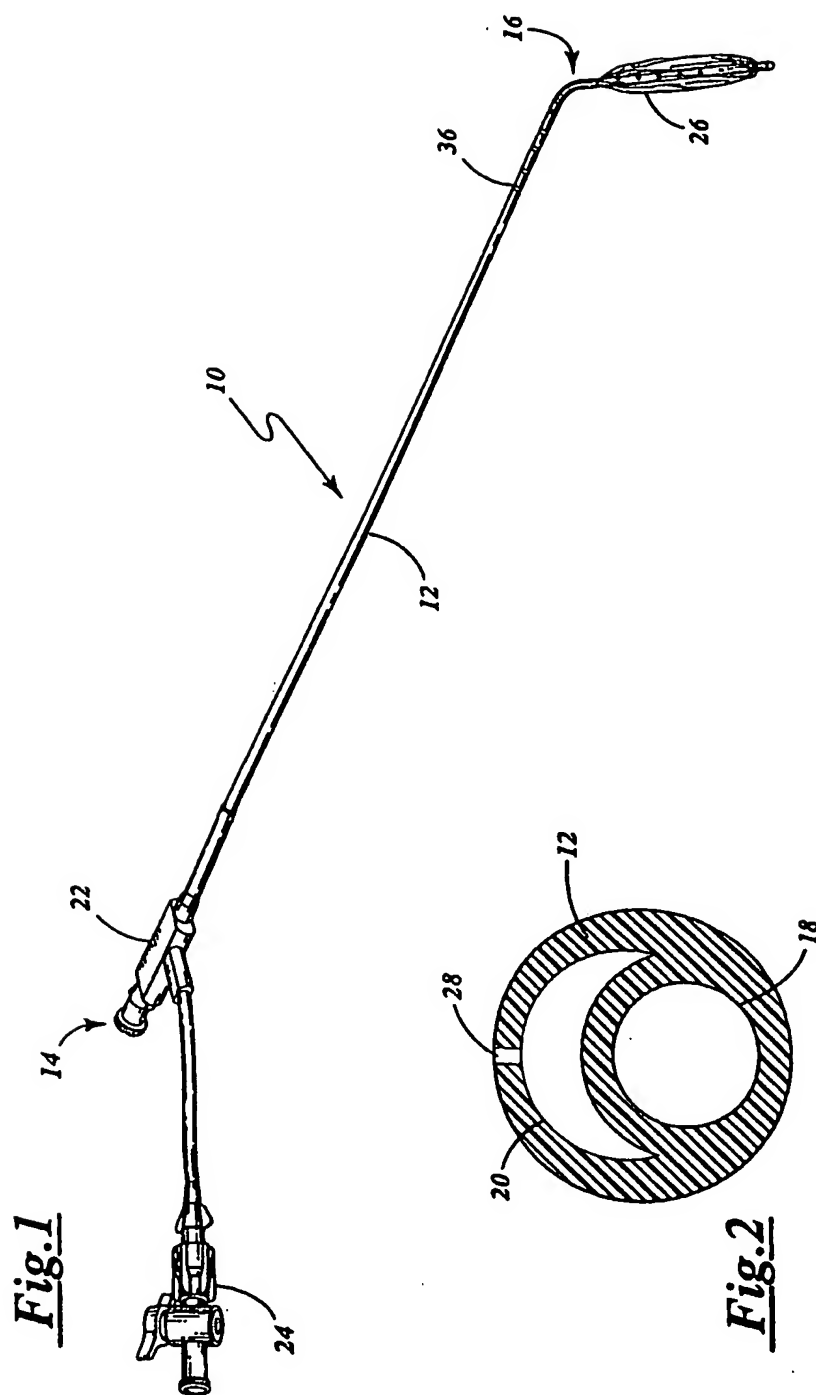

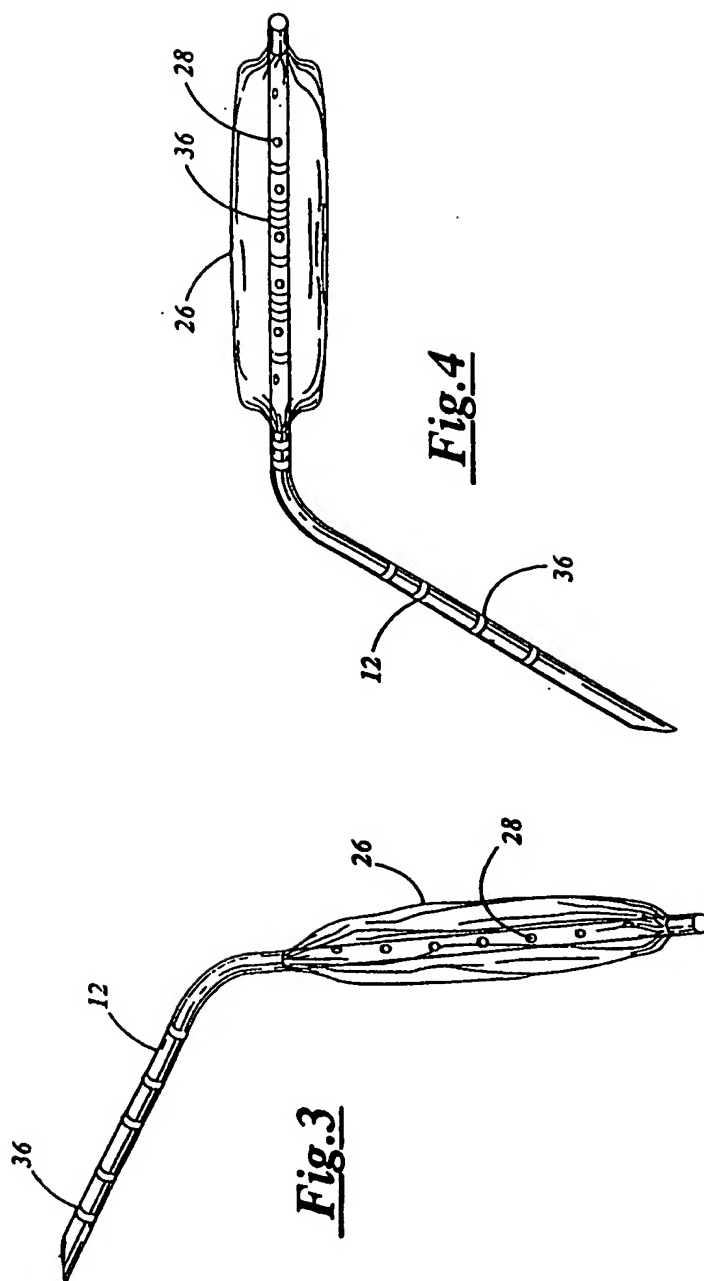

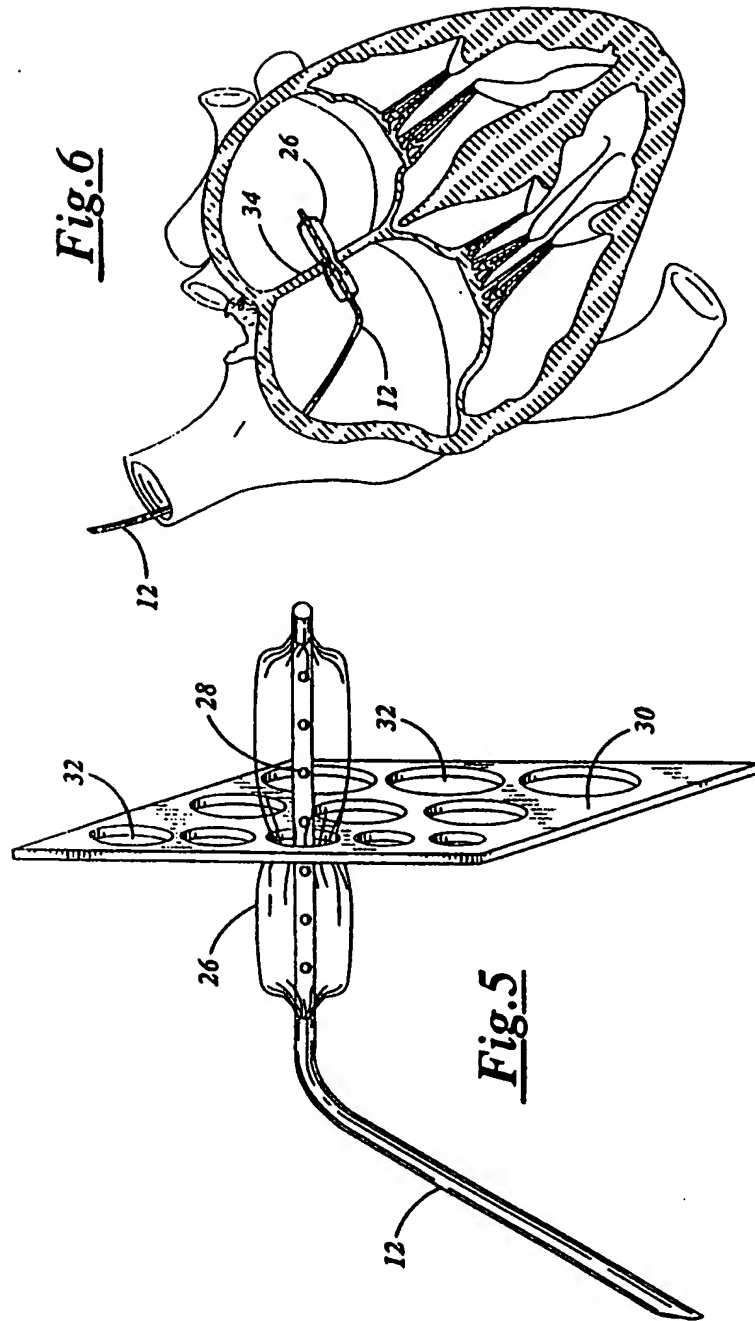
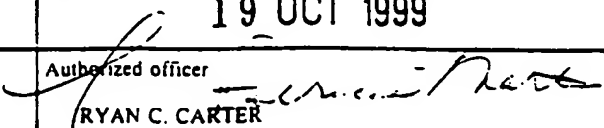


Fig. 7

Model Size(mm)	P. mmHg	Real Size(mm)	Echo Sizing	Difference	Video Sizing	Difference	Cine Sizing	Difference
8	8	7.79	7.91	0.12	7.62	0.18	7.74	0.06
9	10	9.09	8.94	0.15	8.65	0.44	8.41	0.69
10	15	9.93	9.45	0.48	9.71	0.23	9.24	0.69
11	43	11.22	10.8	0.42	10.75	0.47	10.46	0.77
12	50	11.92	11.5	0.42	11.72	0.2	11.52	0.4
13	68	12.72	13.6	0.88	12.54	0.18	12.2	0.53
14	70	14.65	14.5	0.15	14.19	0.47	13.94	0.71
15	88	15.17	16.5	1.33	15.08	0.1	14.47	0.7
16	93	16.03	18	1.97	16.12	0.09	15.45	0.58
17	95	16.8	16.9	0.1	16.87	0.07	16.21	0.18
18	100	18.28	17.3	0.98	18.71	0.43	17.74	0.54
20	120	19.88	19.7	0.18	20.33	0.45	19.35	0.53
22	140	22.3	22.1	0.2	22.74	0.44	21.86	0.45
24	180	24.05	23.6	0.45	24.68	0.63	23.31	0.74
26	200	25.65	26.2	0.55	26.94	1.29	24.84	0.81
28	280	27.06	25.9	1.16	28.55	1.49	26.13	0.93
30	325	30.28	29	1.28	32.1	1.82	29.52	0.77
				average		average		average
				0.64		0.53		0.59
				SD:		SD:		SD:
				0.54		0.52		0.23
					RSQ:		RSQ:	
					0.99886697		0.99932096	

INTERNATIONAL SEARCH REPORT

International application No
PCT/US99/17406

A. CLASSIFICATION OF SUBJECT MATTER IPC(6) :A61B 5/02 US CL :600/481, 508 According to International Patent Classification (IPC) or to both national classification and IPC														
B. FIELDS SEARCHED Minimum documentation searched (classification system followed by classification symbols) U.S. : 600/481, 485, 486, 491, 499, 505, 508, 513; 607/106 Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)														
C. DOCUMENTS CONSIDERED TO BE RELEVANT														
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.												
Y	US 5,591,195 A (TAHERI et al.) 07 January 1997, entire document.	1-11												
A	US 5,269,758 A (TAHERI et al.) 14 December 1993, entire document.	1-11												
<input type="checkbox"/> Further documents are listed in the continuation of Box C. <input type="checkbox"/> See patent family annex.														
<table border="0"> <tr> <td>* Special categories of cited documents</td> <td>*T later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention</td> </tr> <tr> <td>*A* document defining the general state of the art which is not considered to be of particular relevance</td> <td>*X* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone</td> </tr> <tr> <td>*E* earlier document published on or after the international filing date</td> <td>*Y* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art</td> </tr> <tr> <td>*L* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)</td> <td>*A* document member of the same patent family</td> </tr> <tr> <td>*O* document referring to an oral disclosure, use, exhibition or other means</td> <td></td> </tr> <tr> <td>*P* document published prior to the international filing date but later than the priority date claimed</td> <td></td> </tr> </table>			* Special categories of cited documents	*T later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention	*A* document defining the general state of the art which is not considered to be of particular relevance	*X* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone	*E* earlier document published on or after the international filing date	*Y* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art	*L* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	*A* document member of the same patent family	*O* document referring to an oral disclosure, use, exhibition or other means		*P* document published prior to the international filing date but later than the priority date claimed	
* Special categories of cited documents	*T later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention													
A document defining the general state of the art which is not considered to be of particular relevance	*X* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone													
E earlier document published on or after the international filing date	*Y* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art													
L document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	*A* document member of the same patent family													
O document referring to an oral disclosure, use, exhibition or other means														
P document published prior to the international filing date but later than the priority date claimed														
Date of the actual completion of the international search 30 SEPTEMBER 1999		Date of mailing of the international search report 19 OCT 1999												
Name and mailing address of the ISA/US Commissioner of Patents and Trademarks Box PCT Washington, D.C. 20231 Facsimile No. (703) 305-3230		Authorized officer  RYAN C. CARTER Telephone No. (703) 308-2990												